



## The world's most accurate concrete surface resistivity meter


Surface resistivity measurement provides extremely useful information about the state of a concrete structure. Not only has it been proven to be directly linked to the likelihood of corrosion and the corrosion rate, recent studies have shown that there is a direct correlation between resistivity and chloride diffusion rate. The versatility of the method can be seen in these example applications:

- Estimation of the likelihood of corrosion
- Indication of corrosion rate
- Correlation to chloride permeability
- On site assessment of curing efficiency
- Determination of zonal requirements for cathodic protection systems
- Identification of wet and dry areas in a concrete structure
- Indication of variations in the water/cement ratios within a concrete structure
- Identification of areas within a structure most susceptible to chloride penetration
- Correlation to water permeability of rock

Resipod is a fully integrated 4-point Wenner probe, designed to measure the electrical resistivity of concrete in a completely non-destructive test. It is the most accurate instrument available, extremely fast and stable and packaged in a robust, waterproof housing designed to operate in a demanding site environment.





## The measurement principle

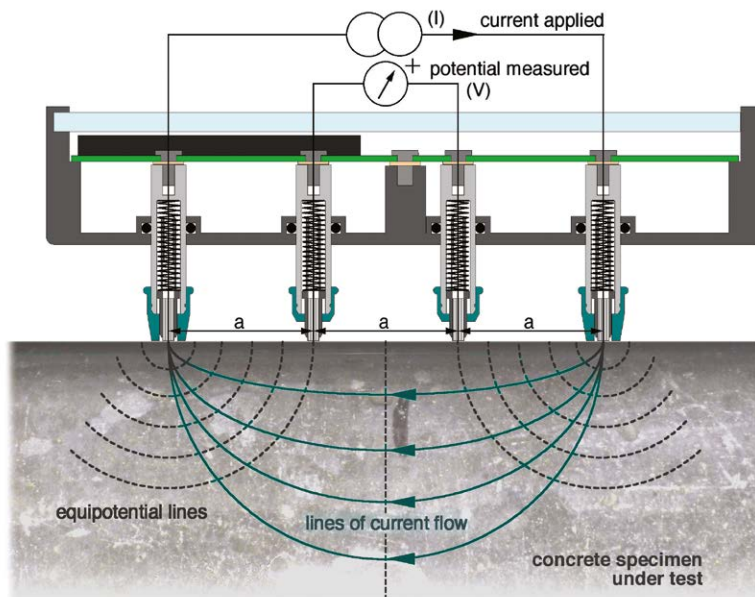

Operating on the principle of the Wenner probe, the Resipod is designed to measure the electrical resistivity of concrete or rock. A current is applied to the two outer probes, and the potential difference is measured between the two inner probes. The current is carried by ions in the pore liquid. The calculated resistivity depends on the spacing of the probes.

$$\text{Resistivity } \rho = 2\pi aV/I \text{ [k}\Omega\text{cm]}$$

## Resipod Models and Probe Spacing

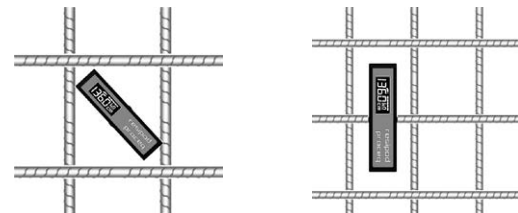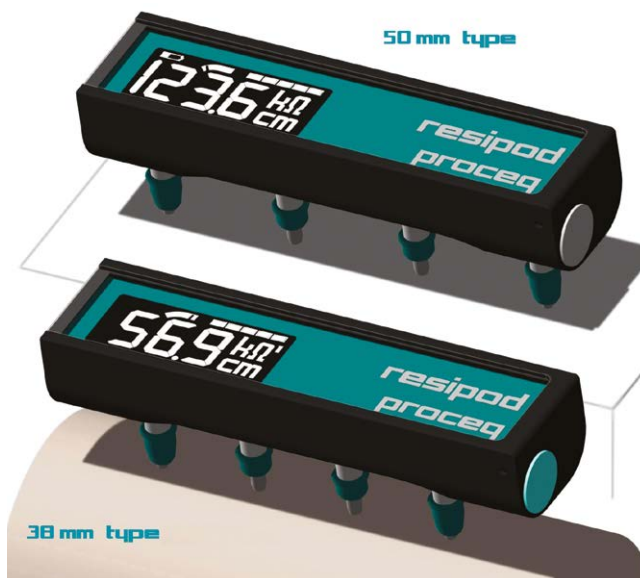

A wider probe spacing provides a more consistent reading when measuring on an inhomogeneous material like concrete. However, if the spacing is too wide, there is more danger of the measurement being affected by the reinforcement steel. The industry standard 50 mm probe spacing has long been seen as a good compromise.

The 38mm (1.5”) model is designed specifically to comply with the AASHTO TP 95-11 standard for “Surface Resistivity Indication of Concrete’s Ability to Resist Chloride Ion Penetration”.

The Surface Resistivity (SR) test is a much quicker and easier test for estimating concrete permeability. It is a proven and mature test method which can replace the more laborious rapid chloride permeability test.


## Unmatched Features

Despite being extremely simple to use, Resipod provides a variety of features that are unique in a concrete surface resistivity instrument.

- Fully integrated surface resistivity instrument
- Wide measuring range (0 to ca. 1000 kΩcm)
- Fast and accurate delivery of measuring results
- Highest resolution available for a surface resistivity instrument
- Meets the AASHTO TP 95-11 standard (38mm, 1.5" probe spacing)
- Current flow indication and poor contact indication
- Hold, save and delete function, with onboard memory
- USB connection and dedicated PC software
- Designed to float (waterproof according to IPX7)
- Allows variable probe spacing to be set
- Allows replacement of standard tips with accessories

## Resipod Display

The display of the Resipod shows all necessary information while acquiring data on site.

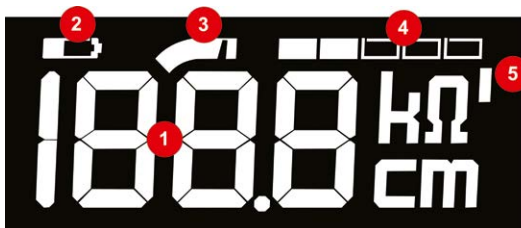

1. Measured resistivity
2. Battery status
3. Range indication
4. Current indication  
20%, 40%, 60%, 80%, 100%
5. Indication of scaled reading

## Indication of poor connection

A good connection between the instrument and the concrete surface is the most important factor for obtaining a reliable measurement. Resipod automatically detects a poor connection and alerts the user.



No contact inner probes




Overflow



“Open Line” indication

## ResipodLink Software

The collected measurement values can then be analyzed comfortably with the Resipod Link PC tool.

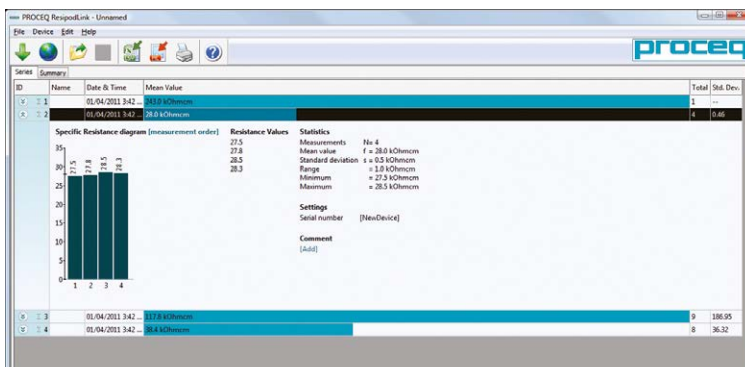

## Technical Information Resipod

Range	0.1 – ca. 1000 kΩcm (depending on probe spacing)
Resolution (nominal current 200μA)	±0.2 kΩcm or ±1% (whichever is greater)
Resolution (nominal current 50μA)	±0.3 kΩcm or ±2% (whichever is greater)
Resolution (nominal current <50μA)	±2 kΩcm or ±5% (whichever is greater)
Frequency	40 Hz
Memory	Non volatile, ca. 500 measured values
Power Supply	>50 hours autonomy
Charger connection	USB type B, (5V, 100mA)
Dimensions	197 x 53 x 69.7 mm (7.8 x 2.1 x 2.7 inch)
Weight	318 g (11.2 oz)
Operating temperature	0° to 50°C (32° to 122°F)
Storage temperature	-10° to 70°C (14° to 158°F)
IP Classification	IP67

## Technical Information Resipod Link software

System requirements: Windows XP, Windows Vista, Windows 7, USB-Connector

An internet connection is necessary for soft- and firmware (using PqUpgrade) updates if available.

## Ordering Information

Units	Description
381 10 000	Resipod, 50mm probe spacing, test strip, foam contact pads, charger with USB-cable, software, carrying strap, documentation and case.
381 20 000	Resipod, 38mm (1.5") probe spacing, test strip, foam contact pads, charger with USB-cable, software, carrying strap, documentation and case.
Parts and Accessories	
381 01 050	Extension cable set
381 01 043S	Set of replacement foam contact pads (20 pieces)
381 01 038	Test strip
381 01 014	USB cover
391 80 110	Carrying strap
341 80 112	USB charger, global

## Service and Warranty Information

Proceq is committed to providing complete support for the Resipod testing instrument by means of our global service and support facilities. Furthermore, each instrument is backed by the standard Proceq 2-year warranty and extended warranty options.

### Standard warranty

Electronic portion of the instrument: 24 months  
Mechanical portion of the instrument: 6 months

### Extended warranty

When acquiring a Resipod, max. 3 additional warranty years can be purchased (for the electronic portion of the instrument). The additional warranty must be requested at time of purchase or within 90 days of purchase.

Subject to change without notice. All information contained in this documentation is presented in good faith and believed to be correct. Proceq SA makes no warranties and excludes all liability as to the completeness and/or accuracy of the information. For the use and application of any product manufactured and/or sold by Proceq SA explicit reference is made to the particular applicable operating instructions.



### Head Office

**Proceq SA**  
Ringstrasse 2  
CH-8603 Schwerzenbach  
Switzerland  
Phone: +41 (0)43 355 38 00  
Fax: +41 (0)43 355 38 12  
info@proceq.com  
www.proceq.com

